



A polyphenol biosensor realized by laser printing technology



Eleftherios Touloupakis^a, Marianneza Chatzipetrou^b, Christos Boutopoulos^b,
Alkisti Gkouzou^b, Ioanna Zergioti^{b,*}

^a Department of Chemistry, University of Crete, Voutes, Heraklion, Crete 71003, Greece

^b Department of Physics, National Technical University of Athens, IroonPolytehneiou 9, Zografou, Athens 15780, Greece

ARTICLE INFO

Article history:

Received 11 June 2013

Received in revised form

12 November 2013

Accepted 26 November 2013

Available online 5 December 2013

Keywords:

Laccase

Phenolic compounds

Biosensor

Immobilization

Laser printing

ABSTRACT

An amperometric biosensor sensitive towards phenolic compounds, using the enzyme laccase as biorecognition element, was developed. The enzyme was successfully immobilized in active form onto nonfunctionalized screen printed electrodes by using the laser printing technology. This type of immobilization established efficient electrochemical contact between the enzyme and the electrodes surface. The immobilized laccase was characterized towards catechol in solution, a typical phenolic compound. The biosensor sensitivity was found to be $0.43\text{nA} \pm 0.04\text{ nA}/\mu\text{M}$ for catechol. This biosensor permits the detection of catechol in aqueous solutions at concentrations in the nanomolar range.

© 2013 Elsevier B.V. All rights reserved.

1. Introduction

Polyphenols are plant-derived natural products with various beneficial properties for the human body [1,2]. This class of molecules exhibits an outstanding performance in the prevention of various human-threatening maladies, from cancer to diabetes, and neurodegenerative diseases. Polyphenols include several thousand compounds such as flavonols, catechins, anthocyanidins, and isoflavonoids [3]; and due to their antioxidant activity they have been widely exploited in the market industry in the form of functional foods, dietary supplements, and anti-aging creams [2,4].

The most used analytical methods for the determination phenolic compounds are GC-MS or HPLC [5]. These methods are expensive and involve complex sample pre-treatment procedure. Many biosensors have been developed as an alternative method using the catalytic activity of the enzymes such as tyrosinase or laccase for phenolic compounds determination [6,7].

Laccases are multicopper oxidoreductases, capable of oxidizing several phenolic and non-phenolic compounds, including polycyclic aromatic hydrocarbons, pesticides, organophosphorus, etc. Widely distributed in higher plants, fungi, and microorganisms [8], laccases can be utilized as a biorecognition element (biomediator) for phenolic compounds in the development of biosensors for

polyphenols detection [9,10], in particular for catechol detection. Amperometric determination of catechol was realized electrochemically by measuring the variation of current signals in the presence of laccase. Since the oxidation of catechol results in benzoquinone, the latter can be electrochemically reduced and detected in a concentration-dependent manner [11].

A large number of techniques have been developed for the immobilization of enzymes for biosensor applications. Generally, the choice of an appropriate immobilization method is determined by the physical and chemical properties of the surface and the biomediator. The most commonly used immobilization methods in biosensing technology are identified either as chemical or physical processes. Chemical immobilization processes are based on covalent attachment while physical immobilization techniques are mainly based on the following mechanisms: adsorption, entrapment, and cross-linking [12,13]. These methods have several disadvantages such as loss of the biological activity, requirement of surface functionalization, are time consuming, use of laborious reactions, and involvement of toxic chemicals.

In our approach, we use the laser induced forward transfer (LIFT) process as an advanced tool for direct immobilization of the enzyme laccase onto low cost nonfunctionalized screen printed electrodes (SPE). This process has been already used for the deposition of enzymes [14], DNA [15], living cells, [16] and photosynthetic membranes [17]. The high spatial resolution of the LIFT process has led several research groups to employ this technique in order to transfer a wide range of biomaterials for the fabrication of biosensors.

* Corresponding author. Tel.: +30 2107723345; fax: +30 2107723025.
E-mail address: zergioti@central.ntua.gr (I. Zergioti).

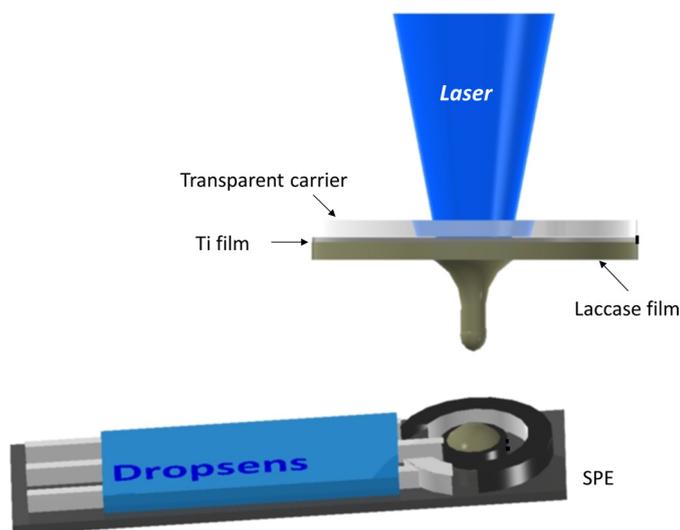


Fig. 1. Schematic illustration of the LIFT process.

This manuscript deals with the use of the LIFT process for the direct laccase immobilization on graphite SPEs for the development of biosensor.

2. Materials and methods

Graphite SPEs (DRP110) were purchased from DropSens (Oviedo, Spain). Laccase from *Trametes versicolor* (E.C.1.10.3.2) was purchased from Sigma–Aldrich (St. Louis, MO USA), claimed activity of at least 0.5 U/mg. All reagents were purchased from Sigma–Aldrich (St. Louis, MO USA) and were of analytical grade.

2.1. Laser printing setup

The laser printing setup is comprised of a pulsed Nd:YAG (neodymium-doped yttrium aluminum garnet) laser (266 nm wavelength, 10 ns pulse duration) and a high power imaging micro-machining system [18]. A donor substrate consists of one inch quartz and 40 nm titanium layer which acts as the dynamic release layer for the laser-assisted process. The liquid film to be deposited is coated to the donor substrate using a microblade and forms a uniform liquid film of 10 μm in thickness.

This method relies on the displacement of the material to be deposited from a donor substrate to an acceptor substrate. Irradiation of the donor substrate results in the rapid heating of the Ti film and the explosive boiling of the adjacent liquid, thus producing a high vapor cavity, which expands and drives through the remaining film. The acceptor substrate is placed parallel to the donor substrate at 300 μm , so that following irradiation, the biomaterial is printed onto the former (Fig. 1).

2.2. Enzyme preparation

Laccase solutions were prepared by dissolving a suitable amount of lyophilized enzyme with known enzymatic activity (40 U), in phosphate buffered saline (PBS) solution pH 4.5. Graphite SPEs DRP110 were used for these experiments, purchased by DropSens, which consist of a counter, a reference, and a working electrode (4 mm diameter). The working electrode was printed with the enzyme (86 mU) in PBS via LIFT technique and afterwards, 50 μL PBS were added for amperometric measurements.

2.3. Biosensor set-up

Tests with the immobilized laccase on the SPEs were performed by using the potentiostat AMPBIO-SPE (Biosensor s.r.l., Rome, Italy; www.biosensor.it). The SPE, with the immobilized enzyme, was polarized at -30 mV relative to an Ag/AgCl reference electrode.

Amperometric detection of the electric current was carried out by the redox reactions taking place in the surface of the working electrode which correspond to the electrochemical oxidation of the catechol and consequently the electrochemical reduction of the generated benzoquinone. Amperometric measurements were carried out at room temperature.

3. Results and discussion

3.1. Laser printing

The direct immobilization of the biomaterials relies on the high velocities that the liquid droplets are being transferred by means of laser printing. The liquid film impacts with high pressure at the rough substrate, resulting in a physical absorption of the biomaterials to the substrate. In this endeavor, the LIFT technique was used for both the deposition and the immobilization of the laccase enzyme onto the surface of commercial graphite SPEs. Two-dimensional patterns of continuous enzyme layers were printed on the electrodes by adjusting the droplet separation distance and size. The transfer was carried out in such a way that each droplet was deposited by a single pulse and a 16×16 array with pixel distance 80 μm resulted to a continuous laccase enzyme film on the electrode. According to the optimum laser transfer conditions, the energy fluence was 400 mJ/cm^2 and the spot size was 75 μm . The physical absorption of the enzyme in the rough substrate was studied by contact angle (CA) measurements. There is a wetting variation in relation to the laser printing energy that can lead to the direct immobilization of the biomaterials on a rough substrate [19] as can be seen in Fig. 2.

As the laser fluence was increased from 125 to 300 mJ/cm^2 , there was a gradual transition from a partial wetting state to a complete wetting state. This is a result of the extremely high impact pressure (1–10 MPa) produced by the high velocity transfer of the biomaterial. The reference partial wetting state obtained by the pipetting method is shown for comparison. The volume of the printed laccase enzyme was calculated through Eq. (1) 1.68 ± 1.61 nL and therefore the concentration of the immobilized laccase enzyme on the graphite SPE was 0.086 ± 0.008 U.

$$V = \frac{\pi h}{6}(3a^2 + h^2) \quad (1)$$

where, a is the radius and h is the height of the printed droplet.

3.2. Biosensor response

In order to evaluate the biosensor performance, tests were conducted on different SPEs with immobilised laccase in the presence of catechol at various concentrations. After a stabilization period the biosensor showed a cathodic current when catechol was added to PBS buffer. Before each test, the SPE was rinsed twice with 50 μL PBS so as to remove any nonphysically absorbed enzyme layers to the graphite SPE. The biosensor showed high signal to noise ratio and in the presence of catechol solution, a reduction current was generated. The reproducibility of the biosensor was good, showing a relative standard deviation (RSD) value of 11.7% and a detection limit of 150 nM. Concerning the repeatability, the biosensor has been used up to four times for the detection of 300 nM catechol solution without a decrease at the amperometric signal response. A dose-response curve was obtained in the presence of several

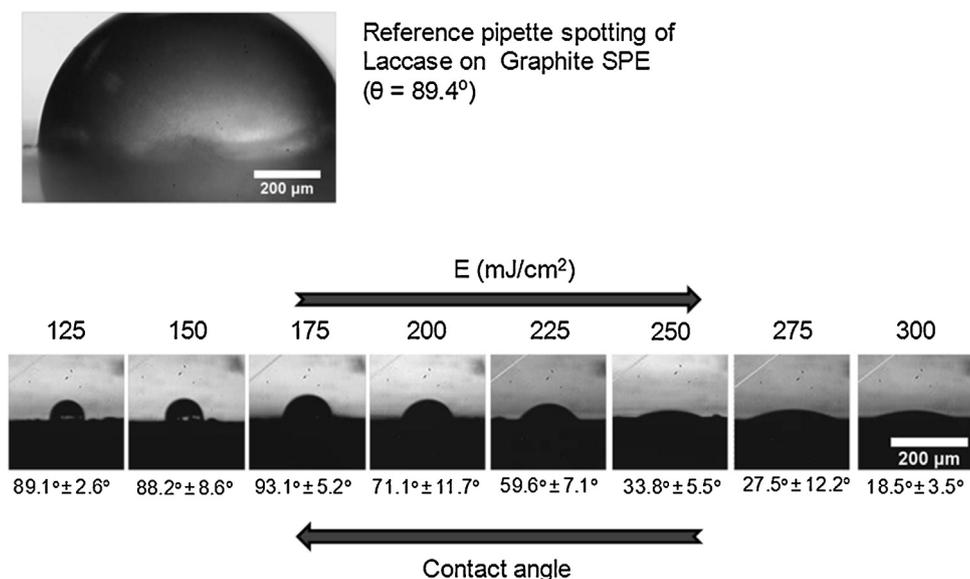


Fig. 2. Optical microscopy images of laccase enzyme liquid droplets deposited on a graphite SPE by the reference pipette method and the LIFT method, respectively.

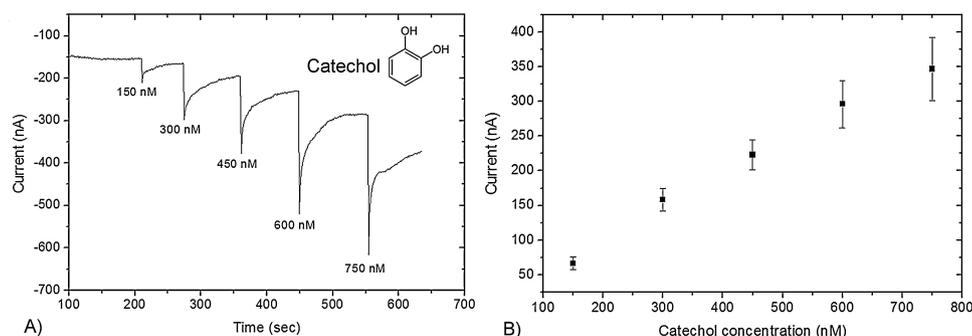


Fig. 3. (A) Response of graphite SPE printed with laccase enzyme via LIFT under various concentrations of catechol (the inset shows the chemical structure of catechol). (B) Standard error of mean value for various concentrations of catechol. Experiments were repeated at least three times.

concentrations of catechol (Fig. 3). The sensitivity for catechol was $0.43 \pm 0.04 \text{ nA}/\mu\text{M}$.

In order to test the specificity of the biosensor, preliminary experiments have shown the LOD of two more phenolic compounds, dopamine, and phenol. The biosensor was able to detect phenol and dopamine with a limit of detection $10 \mu\text{M}$ and 1 mM , respectively. The new analytes were tested under the optimized measuring conditions (pH value, applied potential, etc.), for the detection of catechol. Examples of (A) phenol and (B) dopamine tests are presented in Fig. 4.

Regarding the stability of the biosensor, the response to catechol at different days of storage at 4°C was studied. After 35 days the current response of laccase-SPE reached 90% of the initial response (Fig. 5).

A comparison with similar biosensing devices indicates improved operational features in terms of sensitivity and detection limit (LOD). The advantages of this biosensor rely on the direct immobilization of the laccase enzyme without using toxic reagents that often interfere with, or attenuate, the signal of the analytical device Table 1.

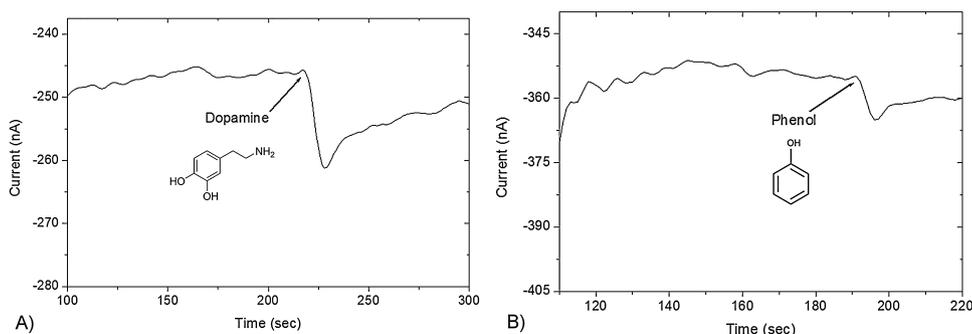


Fig. 4. Relative response of graphite SPE printed with laccase enzyme via LIFT (A) For the detection of dopamine (the inset shows the chemical structure of dopamine) (B) For the detection of phenol (the inset shows the chemical structure of phenol).

Table 1
Comparison of the performance of the actual biosensor and similar devices reported in literature.

Biomediator	Analyte	Sensitivity (nA/ μ M)	LOD (μ M)	Immobilization method	Ref.
Laccase	Catechol	0.43	0.15	Laser printing	This work
Tyrosinase	Catechol	n.d.	1.00	Entrapment	[20]
Laccase	Catechol	210	0.07	Covalent bonding	[21]
Laccase	Catechol	3.02	10.0	Entrapment	[22]

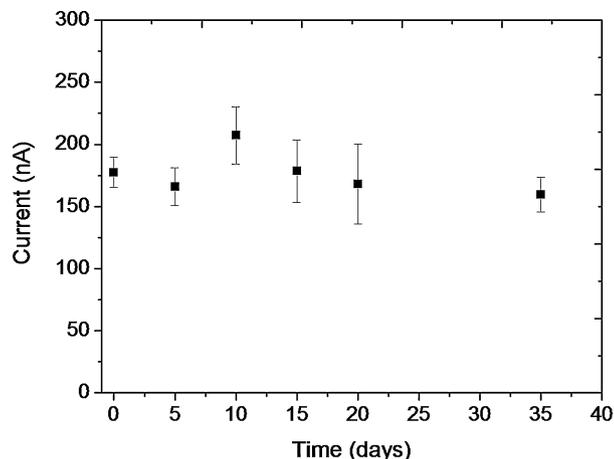


Fig. 5. Storage stability of the biosensor. Tests were performed by using laccase-SPEs in presence of catechol (300 nM).

4. Conclusion

A stable and highly sensitive amperometric laccase based biosensor was developed. Laccase was successfully immobilized in active form on the surface of graphite SPE by using the LIFT technique. The LIFT technique is an advanced tool, not only for the printing the biologic materials, but also for the direct immobilization of them onto rough supports without the need of any type of functionalization. The developed biosensor had a good sensitivity for catechol and, when stored at 4 °C, preserves 90% of activity for 35 days.

Acknowledgements

The authors kindly acknowledge funding from the European Research Council under the European Community's Seventh Framework Program (FP7/2007–2013) COST Action TD1102 Photosynthetic proteins for technological applications: biosensors and biochips (PHOTOTECH) and the, Industry-Academia Partnerships and Pathways Marie Curie action, No 324459, FP7-PEOPLE-2012-IAPP, "LaserMicroFab".

Appendix A. Supplementary data

Supplementary material related to this article can be found, in the online version, at <http://dx.doi.org/10.1016/j.snb.2013.11.110>.

References

- [1] I.C. Arts, P.C. Hollman, Polyphenols and disease risk in epidemiologic studies, *Am. J. Clin. Nutr.* 81 (2005) 317S–325S.
- [2] K.B. Pandey, S.I. Rizvi, Plant polyphenols as dietary antioxidants in human health and disease, *Oxid. Med. Cell. Longev.* 2 (2009) 270–278.
- [3] A.C. Cordova, B.E. Sumpio, Polyphenols are medicine: is it time to prescribe red wine for our patients, *Int. J. Angiol.* 18 (2009) 111–117.
- [4] R.W. Owen, A. Giacosa, W.E. Hull, R. Haubner, B. Spiegelhalter, H. Bartsch, The antioxidant/anticancer potential of phenolic compounds isolated from olive oil, *Eur. J. Cancer.* 36 (2006) 1235–1247.

- [5] R. Maul, N.H. Schyebb, S.E. Kulling, Application of LC and GC hyphenated with mass spectrometry as tool for characterization of unknown derivatives of isoflavonoids, *Anal. Bioanal. Chem.* 391 (2008) 239–250.
- [6] N. Duran, M.A. Rosa, A. D'Annibale, L. Gianfreda, Applications of laccases and tyrosinases (phenoloxidases) immobilized on different supports: a review, *Enzyme Microb. Technol.* 31 (2002) 907–931.
- [7] V. Sanz Carralero, M. Luz Mena, A. Gonzalez-Cortes, P. Yanez-Sedeno, J.M. Pingarron, Development of a tyrosinase biosensor based on gold nanoparticles modified glassy carbon electrodes-application to the measurement of a bio-electrochemical polyphenols index in wines, *Anal. Chim. Acta* 528 (2005) 1–8.
- [8] M. Alcalde, Laccase: biological functions, molecular structure and industrial applications, in: M. Alcalde, J. Polaina (Eds.), *Industrial Enzymes: Structure, Function, and Applications*, Springer, New York, 2007, pp. 459–474.
- [9] Y. Tan, W. Deng, B. Ge, Q. Xie, J. Huang, S. Yao, Biofuel cell and phenolic biosensor based on acid-resistant laccase-glutaraldehyde functionalized chitosan-multiwalled carbon nanotubes nanocomposite film, *Biosens. Bioelectron.* 24 (2009) 2225–2231.
- [10] Y. Li, L. Zhang, M. Li, Z. Pan, D. Li, A disposable biosensor based on immobilization of laccase with silica spheres on the MWCNTs-doped screen-printed electrode, *Chem. Cent. J.* 6 (2012) 103.
- [11] R.C. Minussi, G.M. Pastore, N. Duran, Potential applications of laccase in the food industry, *Trends Food Sci. Technol.* 13 (2002) 205–216.
- [12] Z. Xu, X. Chen, S. Dong, Electrochemical biosensors based on advanced biomobilization matrices, *Trends Anal. Chem.* 25 (2006) 899–908.
- [13] R.A. Sheldon, Enzyme immobilization the quest for optimum performance, *Adv. Synth. Catal.* 349 (2007) 1289–1307.
- [14] P.K. Wu, B.R. Ringeisen, D.B. Krizman, C.G. Frondoza, M. Brooks, D.M. Bubb, R.C.Y. Auyeung, A. Pique, B. Spargo, R.A. McGill, D.B. Chrisey, Laser manipulation of biomaterials: matrix-assisted pulsed-laser evaporation (MAPLE) and MAPLE-direct write (MDW), *Rev. Sci. Instrum.* 74 (2003) 2546–2557.
- [15] M. Chatzipetrou, G. Tsekis, V. Tsouti, S. Chatzandroulis, I. Zergioti, Biosensors by means of the laser induced forward transfer technique, *Appl. Surf. Sci.* (2012), Available online 3 December 2012, ISSN 0169-4332.
- [16] F. Guillemot, A. Souquet, S. Catros, B. Guillotin, J. Lopez, M. Faucon, B. Pippenger, B. Baille, M. Rémy, S. Bellance, P. Chabassier, J.C. Fricain, J. Amédée, High-throughput laser printing of cells and biomaterials for tissue engineering, *Acta Biomater.* 6 (2010) 2494–2500.
- [17] E. Touloupakis, C. Boutopoulos, K. Buonasera, I. Zergioti, M.T. Giardi, A photosynthetic biosensor with enhanced electron transfer generation realized by laser printing technology, *Anal. Bioanal. Chem.* 402 (2011) 3237–3244.
- [18] C. Boutopoulos, C. Pandis, C. Giannakopoulos, P. Pissis, I. Zergioti, Polymer/carbon nanotube composite patterns via laser induced forward transfer, *Appl. Phys. Lett.* 96 (2010) 041104.
- [19] C. Boutopoulos, E. Touloupakis, I. Pezzotti, M.T. Giardi, I. Zergioti, Direct laser immobilization of photosynthetic material on screen printed electrodes for amperometric biosensor, *Appl. Phys. Lett.* 98 (2011) 093703.
- [20] V. Scognamiglio, I. Pezzotti, G. Pezzotti, J. Cano, I. Manfredonia, K. Buonasera, F. Arduini, D. Moscone, G. Palleschi, M.T. Giardi, Towards an integrated biosensor array for simultaneous and rapid multi-analysis of endocrine disrupting chemicals, *Anal. Chim. Acta.* 751 (2012) 161–170.
- [21] D. Quan, W. Shin, Amperometric detection of catechol and catecholamines by immobilized laccase from DeniLite®, *Electroanalysis* 16 (19) (2004) 1576–1582.
- [22] M.R. Montereali, L. Della Seta, W. Vastarella, R. Pilloton, A disposable laccase-tyrosinase based biosensor for amperometric detection of phenolic compounds in must and wine, *J. Mol. Catal. B: Enzym.* 64 (2010) 189–194.

Biographies

Dr. Touloupakis Eleftherios (Visiting Assistant Professor, University of Crete). Graduated in Biological Sciences at the University of Padova (Italy), he received his diploma (M.Sc.) and Doctorate (Ph.D.) in Biochemistry from the University of Crete (Greece). From 2006 to 2009 he worked as postdoctoral fellow on the European project NUTRA-SNACKS at the Department of Chemistry, University of Crete. From 2009 to 2010 he had a postdoctoral research fellowship on the European project BEEP-C-EN at the National Council of Research (Italy).

MSc. M. Chatzipetrou is a Ph.D. student at National Technical University of Athens. She received her diploma in Physics from the University of Patras in 2009 and her diploma thesis was focused on Laser Induced Plasma Spectroscopy. Afterwards she received her Master degree in Micro- and Nano- devices from National Technical University of Athens in 2011 (June) and since then she is a Ph.D. student at the same University. The focus of her research is the laser microprinting of biomaterials for sensors applications.

Dr. Christos Boutopoulos is currently a postdoctoral fellow in the Laser Processing and Plasmonics Laboratory at Ecole Polytechnique de Montreal. He received his B.Sc. in Applied Physics (2005) and his M.Sc. in Microsystems (2008), both from the National Technical University of Athens. In 2011, he received his Ph.D. in Applied Physics from the same university. His Ph.D. work was focused on the development of chemical and biological sensing microsystems by using a laser printing technology. His current research interests involve the use of plasmonics enhanced laser nanosurgery for cells treatment and transfection. He is the first author or co-author of 14 peer-reviewed journal papers dealing with biosensors and laser printing technology.

Alkisti Gkouzou is a Master student at the National Technical University of Athens. She received her B.Sc. Degree in Physics from the University of Patras in 2011, where she focused on the field of Photonics and Optoelectronics. Afterwards, she began working on a M.Sc. Degree in Microsystems and Nanodevices in the Physics Department of NTUA. Her Master Thesis deals with the fabrication of biosensors via laser induced forward transfer (LIFT), with I. Zergioti being her supervisor.

Dr. Ioanna Zergioti (Assistant Professor Physics, National Technical University of Athens) has more than 20 years experience in phenomena related to the interaction of electromagnetic radiation with matter and the development of laser materials processing for applications in nanotechnology and microdevices. During her Ph.D. she worked at the University of California, Berkeley, and after her Ph.D. she did research work at Max Planck Institute fuer Biophysikalische, and then at Philips CFT working on “Stereostiction of passive ceramic electronic 3-Dimensional structures using inkjet and laser sintering technologies”. One of her main research achievement was the use of laser pulses to direct print biomolecules on biosensors and polymers on sensors. She was involved in many Research projects funded by the EC as a Project Coordinator and as Research team member, during the last eighteen years. She has more than 120 publications in International peer reviewed journals and publications in conferences and she has contributed three chapter books on the laser printing technology.